

Safety Instructions

Proline Promass 300

NEPSI: Zone 2



Proline Promass 300

Table of contents

Associated documentation	4
Manufacturer's certificates	5
Manufacturer address	5
Extended order code	5
Safety instructions: General	8
Safety instructions: Installation	9
Temperature tables	10
Connection values: Signal circuits	23

Associated documentation

All documentation is available:

- On the CD-ROM supplied (not included in the delivery for all device versions).
- Available for all device versions via:
 - Internet: www.endress.com/deviceviewer
 - Smart phone/tablet: *Endress+Hauser Operations App*
- In the Download Area of the Endress+Hauser web site: www.endress.com → Download.

This document is an integral part of the following Operating Instructions:

Measuring device	Documentation code			
	HART	FOUNDATION Fieldbus	PROFIBUS PA	PROFIBUS DP
Promass A 300 (8A3B)	BA01482D	BA01515D	BA01504D	–
Promass E 300	BA01484D	BA01517D	BA01506D	BA01855D
Promass F 300	BA01485D	BA01518D	BA01507D	BA01850D
Promass H 300	BA01486D	BA01519D	BA01508D	BA01858D
Promass I 300	BA01487D	BA01520D	BA01509D	BA01859D
Promass O 300	BA01488D	BA01521D	BA01510D	BA01860D
Promass P 300	BA01489D	BA01522D	BA01511D	BA01861D
Promass Q 300	BA01490D	BA01523D	BA01512D	BA01862D
Promass S 300	BA01491D	BA01524D	BA01513D	BA01863D
Promass X 300	BA01492D	BA01525D	BA01514D	BA01864D

Measuring device	Documentation code		
	Modbus RS485	EtherNet/IP	PROFINET
Promass A 300 (8A3B)	BA01493D	BA01699D	BA01736D
Promass E 300	BA01495D	BA01727D	BA01738D
Promass F 300	BA01496D	BA01728D	BA01739D
Promass H 300	BA01497D	BA01729D	BA01740D
Promass I 300	BA01498D	BA01730D	BA01741D
Promass O 300	BA01499D	BA01731D	BA01742D
Promass P 300	BA01500D	BA01732D	BA01743D
Promass Q 300	BA01501D	BA01733D	BA01744D
Promass S 300	BA01502D	BA01734D	BA01745D
Promass X 300	BA01503D	BA01735D	BA01746D

Additional documentation

Contents	Document type	Documentation code
Remote display and operating module DKX001	Special documentation	SD01763D
	Safety Instructions Zone 2; Ex nA	XA01503D
Explosion Protection	Brochure	CP00021Z/11

Manufacturer's certificates**NEPSI Declaration of Conformity**

Certificate number:

GYJ22.1052X

Affixing the certificate number certifies conformity with the following standards (depending on the device version):

- GB3836.1-2010
- GB3836.4-2010
- GB3836.8-2014

Manufacturer address

Endress+Hauser Flowtec AG
Kägenstrasse 7
4153 Reinach BL
Switzerland

Extended order code

The extended order code is indicated on the nameplate, which is affixed to the device in such a way that it is clearly visible. Additional information about the nameplate is provided in the associated Operating Instructions.

Structure of the extended order code

* * * * *	–	* * * * * ... * * * * *	+	A*B*C*D*E*F*G*...
<i>(Device type)</i>		<i>(Basic specifications)</i>		<i>(Optional specifications)</i>

* = Placeholder
At this position, an option (number or letter) selected from the specification is displayed instead of the placeholders.

Device type

The device and the device design is defined in the "Device type" section (Product root).

Basic specifications

The features that are absolutely essential for the device (mandatory features) are specified in the basic specifications. The number of positions depends on the number of features available. The selected option of a feature can consist of several positions.

Optional specifications

The optional specifications describe additional features for the device (optional features). The number of positions depends on the number of features available. The features have a 2-digit structure to aid identification (e.g. JA). The first digit (ID) stands for the feature group and consists of a number or a letter (e.g. J = Test, Certificate). The second digit constitutes the value that stands for the feature within the group (e.g. A = 3.1 material (wetted parts), inspection certificate).

More detailed information about the device is provided in the following tables. These tables describe the individual positions and IDs in the extended order code which are relevant to hazardous locations.

Device type

Position	Order code for	Option selected	Description
1	Instrument family	B	Coriolis flowmeter
2	Sensor	A, E, F, H, I, O, P, Q, S, X	Sensor type
3	Transmitter	3	Transmitter type: 4-wire, compact version
4	Generation index	B, C	Platform generation
5, 6	Nominal diameter	DN 1 ... 350 DN 1: 01 DN 2: 02 ... DN 350: 3E, 3F, 3R	Nominal diameter of sensor

Basic specifications

Position 1, 2 Order code for "Approval" Option selected	Type of protection	
	Transmitter	Sensor
NS	Ex nA nC IIC T1~T5 Gc	Ex nA IIC T1~T5 Gc
	Ex nA nC [ic] IIC T1~T5 Gc ²⁾	Ex nA nC IIC T1~T5 Gc ¹⁾

- 1) Sensors with type of protection Ex nA nC are only available for sensor versions without purge connection or rupture disk (see "Optional specifications")
- 2) The marking Ex nA nC [ic] IIC T1~T5 Gc is only available for devices with order code "Output; Input 1", option HA or TA

Position	Order code for	Option selected	Description
4, 5	Output, input 1	BA	4-20mA HART
		GA	PROFIBUS PA
		HA	PROFIBUS PA Ex-i
		LA	PROFIBUS DP
		MA	Modbus RS485
		NA	EtherNet/IP 2-port switch integrated
		RA	PROFINET IO 2-port switch integrated
		SA	FOUNDATION Fieldbus
		TA	FOUNDATION Fieldbus Ex-i
6	Output, input 2	A	W/o
		B	4-20mA
		C	4-20mA Ex-i passive
		D	Configurable I/O initial setting off
		E	Pulse/frequency/switch output
		F	Pulse output, phase-shifted
		G	Pulse/frequency/switch output Ex-i passive
		H	Relay
		I	4-20mA input
		J	Status input
7	Output, input 3	A	W/o
		B	4-20mA
		C	4-20mA Ex-i passive
		D	Configurable I/O initial setting off
		E	Pulse/frequency/switch output
		F	Pulse output, phase-shifted
		G	Pulse/frequency/switch output Ex-i passive
		H	Relay
		I	4-20mA input
		J	Status input
8	Display; Operation	A	W/o; via communication
		F	4-line, illuminated; touch control
		G	4-line, illuminated; touch control + WLAN
		M	W/o; prepared for remote display DKX001

Position	Order code for	Option selected	Description
		O	Separate, with remote display DKX001, 4-line, illuminated; 10 m / 30 ft cable; touch control
9	Housing	A	Alu, coated
		B	Stainless, hygienic
		L	Cast, stainless
11, 12	Meas. Tube Mat., Wetted Parts Surface	LA	Stainl. steel, cryogenic -196°C/-320°F
17, 18	Device Model	A1	1
		A2	2

Optional specifications

ID	Order code for	Option selected	Description
Cx	Sensor option	CA	Rupture disk
Cx	Sensor option	CH	Purge connection
Px	Enclosed accessories	P8	Wireless antenna, wide area (external WLAN antenna) ¹⁾


1) The external WLAN antenna is available with the order code for "Accessory Enclosed", option P8.

Safety instructions: General

- Staff must meet the following conditions for mounting, electrical installation, commissioning and maintenance of the device:
 - Be suitably qualified for their role and the tasks they perform
 - Be trained in explosion protection
 - Be familiar with national regulations or guidelines (e.g. GB/T 3836.15-2017)
- Install the device according to the manufacturer's instructions and the following standards:
 - GB50257-2014 "Code for construction and acceptance of electric device for explosive atmospheres and fire hazard electrical equipment installation engineering"
 - GB3836.13-2013 "Explosive atmospheres – Part 13: Equipment repair, overhaul and reclamation"
 - GB/T3836.15-2017 "Explosive atmospheres – Part 15: Electrical installations design, selection and erection"
 - GB/T3836.16-2017 "Explosive atmospheres – Part 16: Electrical installations inspection and maintenance"
 - GB/T3836.18-2017 "Explosive atmospheres – Part 18: Intrinsically safe electrical systems"
- Do not operate the device outside the specified electrical, thermal and mechanical parameters.

- Only use the device in media to which the wetted materials have sufficient durability.
- Refer to the temperature tables for the relationship between the permitted ambient temperature for the sensor and/or transmitter, depending on the range of application, and the temperature classes.
- Modifications to the device can affect the explosion protection and must be carried out by staff authorized to perform such work by Endress+Hauser.
- Observe all the technical data of the device (see nameplate).

Safety instructions: Installation

- In the case of a horizontal orientation and the order code for "Housing", option B "Stainless, hygienic": install the transmitter at the side of or below the sensor.
For more information on the orientation, see the Operating Instructions for the device →  4
- The following applies for devices with order code for "Housing", Option B "Stainless, hygienic": Thermal insulation is not allowed.
- Continuous service temperature of the connecting cable: -40 to +80 °C; in accordance with the range of service temperature taking into account additional influences of the process conditions ($T_{a,min}$ and $T_{a,max} + 20$ K).
- Only use certified cable entries suitable for the application. Observe selection criteria as per GB/T3836.15-2017.
- When the measuring device is connected, attention must be paid to explosion protection at the transmitter.
- Turning the transmitter housing
 - Loosen both hexagon socket screws until the transmitter housing can be turned.
 - Turn transmitter housing to desired position (mechanically limited); if necessary turn 270° in other direction.
 - Tighten both hexagon socket screws with a maximum of 7 Nm.
- In potentially explosive atmospheres:
 - Do not disconnect the electrical connection of the power supply circuit when energized.
 - Do not open the connection compartment cover when energized.

Ex nA type of protection

- In potentially explosive atmospheres: Do not disconnect the electrical connection of the power supply circuit when energized.
- Seal unused entry glands with approved sealing plugs that correspond to the type of protection.
- Only use certified cable entries or sealing plugs.
- Equipment in type of protection Ex nA, shall be installed using a transient protection not exceeding 140% of the peak rated voltage value at the power supply terminals and IO terminals.
- For measuring devices with order code "Housing", option B "Stainless, hygienic" tighten the connection compartment cover hand-tight and then tighten it further 45° (corresponds to 15 Nm).

Optional external WLAN antenna

- Connect the antenna bushing H337 to the transmitter housing and tighten by hand.
- Use only external antennas supplied by Endress+Hauser.
- Connect antenna or antenna cable with plug-in connector type N (MIL-STD-348) to antenna bushing H337.

Intrinsic safety

Observe the guidelines for interconnecting intrinsically safe circuits (e.g. GB/T 3836.15-2017 , Proof of Intrinsic Safety).



- When using the remote display and operating module DKX001 the internal display and operating module must be removed.
- When using the separate approved, remote display and operating module DKX001, only use the following variants: Basic specification of the remote display and operating module DKX001, order code "Approval", option NS

Potential equalization

- Integrate the device into the local potential equalization .
- If the ground connection has been established via the pipe as specified, it is also possible to integrate the sensor into the potential equalization system via the pipe.
- The antenna bushing H337 of the external antenna must be integrated into the local potential equalization system. This is the case if the sensor is connected in accordance with the regulations via the coupling.

Temperature tables

Ambient temperature

Minimum ambient temperature

$$T_a = -40\text{ °C}$$

Maximum ambient temperature

$T_a = +60\text{ °C}$ depending on the medium temperature and temperature class.

Medium temperature

Minimum medium temperature

- Promass A, F, H, I, P, Q, S, X:
 $T_m = -50\text{ °C}$
- Promass E, O:
 $T_m = -40\text{ °C}$
- Promass F, Q with cryogenic temperature version (order code for "Measuring tube material", option LA):
 $T_m = -196\text{ °C}$

Maximum medium temperature

- T_m for T1 ~ T5 depending on the maximum ambient temperature T_a
- () = The maximum permitted medium temperatures in brackets only apply if the sensor is installed in such a way that the transmitter is not mounted above the sensor and free convection can occur on all sides.

Compact version

NOTICE

In case of heating, risk of overheating.

- ▶ On devices with Heating jacket the corresponding temperature tables for isolated sensor, are to be observed.
- ▶ Make sure that the heating medium, may not exceeded the maximum specified medium temperature of the exact used temperature classes of the device.

Maximum medium temperature without thermal insulation according to Endress+Hauser specifications

Promass A (8A3B**-*..., 8A3C**-*...)

DN	T_a [°C]	$T_{m,max}$ [°C]	T_m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
1...4	50	205	-	90 ^{1) 2)}	130	170 ³⁾	205	205
	60		-	-	130	170 ³⁾	205	205

- 1) The following applies for sensors with type of protection Ex nA nC: $T_m = 95\text{ °C}$
- 2) The maximum admissible ambient temperature changes for devices with order code for "Housing", Option B "Stainless, hygienic" in connection with temperature class T5: $T_a = T_m - 3\text{ K}$
- 3) The following applies for sensors with type of protection Ex nA nC: $T_m = 195\text{ °C}$

Promass E

DN	T _a [°C]	T _{m,max} [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
8...15	50	150	–	80 ^{1) 2)}	115 ³⁾	150	150	150
	55		–	–	115 ³⁾	150	150	150
	60		–	–	(115 ³⁾)	(140 ⁴⁾)	(150)	(150)
25...80	50	150	–	80 ^{1) 2)}	95 ³⁾	140 ⁴⁾	150	150
	55		–	–	95 ³⁾	140 ⁴⁾	150	150
	60		–	–	(95 ³⁾)	(140 ⁴⁾)	(150)	(150)

- 1) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 2) The maximum admissible ambient temperature changes for devices with order code for "Housing", Option B "Stainless, hygienic" in connection with temperature class T5: T_a = T_a - 3 K
- 3) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C
- 4) The following applies for sensors with type of protection Ex nA nC: T_m = 150 °C

Promass F

DN	T _a [°C]	T _{m,max} ¹⁾ [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
08...15	50	150	–	80 ^{2) 3)}	115 ⁴⁾	150	150	150
	60		–	–	115 ⁴⁾	150	150	150
	50	150 ⁵⁾	–	80 ^{2) 3)}	100	150	150	150
	55		–	–	100	150	150	150
	60		–	–	100	150	150	150
	50	240	–	80 ^{2) 3)}	115 ⁴⁾	170 ⁶⁾	240	240
	55		–	–	115 ⁴⁾	170 ⁶⁾	240	240
	60		–	–	115 ⁴⁾	170 (240)	170 (240)	
25...80	50	150	–	60 ^{2) 3)}	95 ⁴⁾	150	150	150
	60		–	–	95 ⁴⁾	150	150	150
	50	150 ⁵⁾	–	60 ^{2) 3)}	95	150	150	150
	55		–	–	95	150	150	150
	60		–	–	95	150	150	150
	50	240	–	60 ^{2) 3)}	95 ⁴⁾	160 ⁶⁾	240	240
	55		–	–	95 ⁴⁾	160 ⁶⁾	240	240

DN	T _a [°C]	T _{m, max} ¹⁾ [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
	60		-	-	95 ⁴⁾	150 ⁷⁾	170 (240)	170 (240)
15, 25, 50... 250	50	350	-	85 ^{2) 3)}	120 ⁴⁾	185 ⁶⁾	280 ⁸⁾	350
	60		-	-	120 ⁴⁾	185 ⁶⁾	280 ⁸⁾	350
100...250	50	150	-	60 ^{2) 3)}	95 ⁴⁾	150	150	150
	60		-	-	95 ⁴⁾	150	150	150
	50	150 ⁵⁾	-	60 ^{2) 3)}	95	150	150	150
	60		-	-	95	150	150	150
	50	240	-	60 ^{2) 3)}	95 ⁴⁾	160 ⁶⁾	240	240
	55		-	-	95 ⁴⁾	160 ⁶⁾	240	240
	60		-	-	95 ⁴⁾	160 ⁷⁾	170 (240)	170 (240)

- 1) Maximum temperature range, see nameplate
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 3) The maximum admissible ambient temperature changes for devices with order code for "Housing", Option B "Stainless, hygienic" in connection with temperature class T5: T_a = T_a - 3 K
- 4) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C
- 5) Cryogenic temperature version: T_m = -196 to 150 °C
- 6) The following applies for sensors with type of protection Ex nA nC: T_m = 195 °C
- 7) The following applies for sensors with type of protection Ex nA nC: T_m = 170 °C
- 8) The following applies for sensors with type of protection Ex nA nC: T_m = 290 °C

Promass H

DN	T _a [°C]	T _{m, max} ¹⁾ [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
8	50	150	-	80 ²⁾	115 ³⁾	150	150	150
	60		-	-	115 ³⁾	150	150	150
8	50	205	-	80 ²⁾	115 ³⁾	165 ⁴⁾	205	205
	60		-	-	115 ³⁾	165 ⁴⁾	205	205
15...50	50	150	-	60 ²⁾	95 ³⁾	130 ⁵⁾	150	150
	60		-	-	95 ³⁾	130 ⁵⁾	150	150

DN	T _a [°C]	T _{m,max} ¹⁾ [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
15...50	50	205	-	60 ²⁾	95 ³⁾	130 ⁴⁾	205	205
	60		-	-	95 ³⁾	130 ⁴⁾	205	205

- 1) Maximum temperature range, see nameplate
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 3) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C
- 4) The following applies for sensors with type of protection Ex nA nC: T_m = 195 °C
- 5) The following applies for sensors with type of protection Ex nA nC: T_m = 150 °C

Promass I

DN	T _a [°C]	T _{m,max} [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
8...80	50	150	-	60 ^{1) 2)}	95 ³⁾	150	150	150
	55		-	-	95 ³⁾	150	150	150
	60		-	-	(95 ³⁾)	(150)	(150)	(150)

- 1) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 2) The maximum admissible ambient temperature changes for devices with order code for "Housing", Option B "Stainless, hygienic" in connection with temperature class T5: T_a = T_m - 3 K
- 3) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C

Promass O

DN	T _a [°C]	T _{m,max} [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
80 ... 250	50	205	-	60 ¹⁾	95 ²⁾	160 ³⁾	205	205
	55		-	-	95 ²⁾	160 ³⁾	205	205
	60		-	-	95 ²⁾	160 ⁴⁾	180 (205)	180 (205)

- 1) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C
- 3) The following applies for sensors with type of protection Ex nA nC: T_m = 195 °C
- 4) The following applies for sensors with type of protection Ex nA nC: T_m = 180 °C

Promass P

DN	T _a [°C]	T _{m, max} ¹⁾ [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
8	50	150	–	80 ^{2) 3)}	115 ⁴⁾	150	150	150
	60		–	–	115 ⁴⁾	150	150	150
	50	205	–	80 ^{2) 3)}	115 ⁴⁾	170 ⁵⁾	205	205
	60		–	–	115 ⁴⁾	170 ⁵⁾	205	205
15...50	50	150	–	60 ^{2) 3)}	95 ⁴⁾	150	150	150
	60		–	–	95 ⁴⁾	150	150	150
	50	205	–	60 ^{2) 3)}	95 ⁴⁾	160 ⁵⁾	205	205
	60		–	–	95 ⁴⁾	160 ⁵⁾	205	205

- 1) Maximum temperature range, see nameplate
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 3) The maximum admissible ambient temperature changes for devices with order code for "Housing", Option B "Stainless, hygienic" in connection with temperature class T5: T_a = T_a - 3 K
- 4) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C
- 5) The following applies for sensors with type of protection Ex nA nC: T_m = 195 °C

Promass Q

DN	T _a [°C]	T _{m, max} ¹⁾ [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
25 ... 100	50	205	–	60 ^{2) 3)}	95 ⁴⁾	160 ⁵⁾	205	205
	60		–	–	95 ⁴⁾	160 ⁵⁾	205	205
25 ... 100	50	150 ⁶⁾	–	60 ^{2) 3)}	95 ⁴⁾	150	150	150
	60		–	–	95 ⁴⁾	150	150	150

- 1) Maximaler Temperaturbereich siehe Typenschild
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 3) The maximum admissible ambient temperature changes for devices with order code for "Housing", Option B "Stainless, hygienic" in connection with temperature class T5: T_a = T_a - 3 K
- 4) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C
- 5) The following applies for sensors with type of protection Ex nA nC: T_m = 195 °C
- 6) Cryogenic temperature version: T_m = -196 to 150 °C

Promass S

DN	T _a [°C]	T _{m,max} [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
8	50	150	–	80 ^{1) 2)}	115 ³⁾	150	150	150
	60		–	–	115 ³⁾	150	150	150
15...50	50	150	–	60 ^{1) 2)}	95 ³⁾	150	150	150
	60		–	–	95 ³⁾	150	150	150

- 1) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 2) The maximum admissible ambient temperature changes for devices with order code for "Housing", Option B "Stainless, hygienic" in connection with temperature class T5: T_a = T_a - 3 K
- 3) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C

Promass X

DN	T _a [°C]	T _{m,max} [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
350	50	180	–	60 ¹⁾	95 ²⁾	160 ³⁾	180	180
	55		–	–	95 ²⁾	160 ³⁾	180	180
	60		–	–	(95 ²⁾)	(160 ³⁾)	(180)	(180)

- 1) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C
- 3) The following applies for sensors with type of protection Ex nA nC: T_m = 180 °C

Maximum medium temperature with thermal insulation according to Endress+Hauser specifications

NOTICE

The following applies for devices with order code for "Housing", Option B "Stainless, hygienic":

- Thermal insulation is not allowed.



For information on the thermal insulation of the device, see the "Thermal insulation" section of the "Operating instructions" document.

Promass A (8A3B**-*..., 8A3C**-*...)

DN	T _a [°C]	T _{m, max} [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
1...4	50	205	-	90 ¹⁾	130	170 ²⁾	205	205
	55		-	-	(130)	(170 ²⁾)	(205)	(205)

- 1) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 195 °C

Promass E

DN	T _a [°C]	T _{m, max} [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
8...15	50	150	-	80 ¹⁾	115 ²⁾	150	150	150
	55		-	-	(115 ²⁾)	(140 ³⁾)	(150)	(150)
25...80	50	150	-	60 ¹⁾	95 ²⁾	140 ³⁾	150	150
	55		-	-	(95 ²⁾)	(140 ³⁾)	(150)	(150)

- 1) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C
- 3) The following applies for sensors with type of protection Ex nA nC: T_m = 150 °C

Promass F

DN	T _a [°C]	T _{m, max} ¹⁾ [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
08...15	50	150	-	80 ²⁾	115 ³⁾	150	150	150
	55		-	-	(115 ³⁾)	(150)	(150)	(150)
	50	150 ⁴⁾	-	80	100	150	150	150

DN	T _a [°C]	T _{m,max} ¹⁾ [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
	55	240	-	-	100	150	150	150
	50		-	80 ²⁾	115 ³⁾	170 ⁵⁾	240	240
	55		-	-	(115 ³⁾)	(170 ⁵⁾)	(240)	(240)
25...80	50	150	-	60 ²⁾	95 ³⁾	150	150	150
	55		-	-	(95 ³⁾)	(150)	(150)	(150)
	50	150 ⁴⁾	-	60 ²⁾	95	150	150	150
	55		-	-	95	150	150	150
	50	240	-	60 ²⁾	95 ³⁾	160 ⁵⁾	240	240
	55		-	-	(95 ³⁾)	(160 ⁵⁾)	(240)	(240)
15, 25, 50... 250	50	350	-	85 ²⁾	120 ³⁾	185 ⁵⁾	280 ⁶⁾	350
	60		-	-	120 ³⁾	185 ⁵⁾	280 ⁶⁾	350
100...250	50	150	-	60 ²⁾	95 ³⁾	150	150	150
	55		-	-	(95 ³⁾)	(150)	(150)	(150)
	50	150 ⁴⁾	-	60 ²⁾	95	150	150	150
	55		-	-	95	150	150	150
	50	240	-	60 ²⁾	95 ³⁾	160 ⁵⁾	240	240
	55		-	-	(95 ³⁾)	(160 ⁵⁾)	(240)	(240)

1) Maximum temperature range, see nameplate

2) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C

3) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C

4) Cryogenic temperature version: T_m = -196 to 150 °C

5) The following applies for sensors with type of protection Ex nA nC: T_m = 195 °C

6) The following applies for sensors with type of protection Ex nA nC: T_m = 290 °C

Promass H

DN	T _a [°C]	T _{m,max} ¹⁾ [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
8	50	150	-	80 ²⁾	115 ³⁾	150	150	150
	55		-	-	(115 ³⁾)	(150)	(150)	(150)
8	50	205	-	80 ²⁾	115 ³⁾	165 ⁴⁾	205	205
	55		-	-	(115 ³⁾)	(165 ⁴⁾)	(205)	(205)
15...50	50	150	-	60 ²⁾	95 ³⁾	130 ⁵⁾	150	150

DN	T _a [°C]	T _{m, max} ¹⁾ [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
	55		-	-	(95 ³⁾)	(130 ⁵⁾)	(150)	(150)
15...50	50	205	-	60 ²⁾	95 ³⁾	130 ⁴⁾	205	205
	55		-	-	(95 ³⁾)	(130 ⁴⁾)	(205)	(205)

- 1) Maximum temperature range, see nameplate
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 3) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C
- 4) The following applies for sensors with type of protection Ex nA nC: T_m = 195 °C
- 5) The following applies for sensors with type of protection Ex nA nC: T_m = 150 °C

Promass I

DN	T _a [°C]	T _{m, max} [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
8...80	50	150	-	60 ¹⁾	95 ²⁾	150	150	150
	60		-	-	(95 ²⁾)	(150)	(150)	(150)

- 1) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C

Promass O

DN	T _a [°C]	T _{m, max} [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
80 ... 250	50	205	-	60 ¹⁾	95 ²⁾	160 ³⁾	205	205
	55		-	-	(95 ²⁾)	(160 ³⁾)	(205)	(205)

- 1) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C
- 3) The following applies for sensors with type of protection Ex nA nC: T_m = 195 °C

Promass P

DN	T _a [°C]	T _{m, max} ¹⁾ [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
8	50	150	-	80 ²⁾	115 ³⁾	150	150	150
	55		-	-	(115 ³⁾)	(150)	(150)	(150)
	50	205	-	80 ²⁾	115 ³⁾	170 ⁴⁾	205	205

DN	T _a [°C]	T _{m,max} ¹⁾ [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
	55		–	–	(115 ³⁾)	(170 ⁴⁾)	(205)	(205)
15...50	50	150	–	60 ²⁾	95 ³⁾	150	150	150
	55		–	–	95 ³⁾	150	150	150
	60		–	–	(95 ³⁾)	(150)	(150)	(150)
	50	205	–	60 ²⁾	95 ³⁾	160 ⁴⁾	205	205
	55		–	–	95 ³⁾	160 ⁴⁾	205	205
	60		–	–	(95 ³⁾)	(160 ⁴⁾)	(205)	(205)

- 1) Maximum temperature range, see nameplate
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 3) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C
- 4) The following applies for sensors with type of protection Ex nA nC: T_m = 195 °C

Promass Q

DN	T _a [°C]	T _{m,max} ¹⁾ [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
25 ... 100	50	205	–	60 ²⁾	95 ³⁾	160 ⁴⁾	205	205
	55		–	(40)	(95)	(160)	(205)	(205)
25 ... 100	50	150 ⁵⁾	–	60 ²⁾	95 ³⁾	150	150	150
	55		–	(40)	(95)	(150)	(150)	(150)

- 1) Maximum temperature range, see nameplate
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 3) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C
- 4) The following applies for sensors with type of protection Ex nA nC: T_m = 195 °C
- 5) Cryogenic temperature version: T_m = –196 to 150 °C

Promass S

DN	T _a [°C]	T _{m,max} [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
8	50	150	–	80 ¹⁾	115 ²⁾	150	150	150
	55		–	–	(115 ²⁾)	(150)	(150)	(150)
15...50	50	150	–	60 ¹⁾	95 ²⁾	150	150	150

DN	T _a [°C]	T _{m, max} [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
	55		-	-	95 ²⁾	150	150	150
	60		-	-	(95 ²⁾)	(150)	(150)	(150)

- 1) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C

Promass X

DN	T _a [°C]	T _{m, max} [°C]	T _m [°C]					
			T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
350	50	180	-	60 ¹⁾	95 ²⁾	160 ³⁾	180	180
	55		-	-	(95 ²⁾)	(160 ³⁾)	(180)	(180)


- 1) The following applies for sensors with type of protection Ex nA nC: T_m = 95 °C
- 2) The following applies for sensors with type of protection Ex nA nC: T_m = 130 °C
- 3) The following applies for sensors with type of protection Ex nA nC: T_m = 180 °C

With thermal insulation without Endress+Hauser specifications

NOTICE


The following applies for devices with order code for "Housing", Option B "Stainless, hygienic":

- Thermal insulation is not allowed.


 For information on the thermal insulation of the device, see the "Thermal insulation" section of the "Operating instructions" document.

The specified reference temperature T_{ref} and the maximum medium temperature $T_{m, max}$ for each temperature class must not be exceeded.

→  17

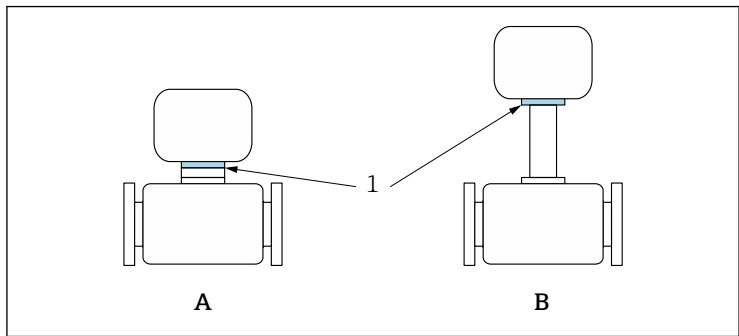

A0031198

 1 Position of reference point for temperature measurement

A Standard version

B Extended temperature version, cryogenic temperature version, high-temperature version

1 Reference point (T_{ref})

Reference temperature T_{ref}

T_m [°C]					
T6 [85 °C]	T5 [100 °C]	T4 [135 °C]	T3 [200 °C]	T2 [300 °C]	T1 [450 °C]
-	63	72	75	77	77

Connection values: Signal circuits

The following tables contain specifications which are dependent on the transmitter type and its input and output assignment. Compare the following specifications with those on the nameplate of the transmitter.

Terminal assignment

Transmitter: supply voltage, input/outputs

HART

Supply voltage		Input/output 1		Input/output 2		Input/output 3	
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (+)	23 (-)
Device-specific terminal assignment: adhesive label in terminal cover.							

FOUNDATION Fieldbus

Supply voltage		Input/output 1		Input/output 2		Input/output 3	
1 (+)	2 (-)	26 (A)	27 (B)	24 (+)	25 (-)	22 (+)	23 (-)
Device-specific terminal assignment: adhesive label in terminal cover.							

PROFIBUS PA

Supply voltage		Input/output 1		Input/output 2		Input/output 3	
1 (+)	2 (-)	26 (B)	27 (A)	24 (+)	25 (-)	22 (+)	23 (-)
Device-specific terminal assignment: adhesive label in terminal cover.							

PROFIBUS DP

Supply voltage		Input/output 1		Input/output 2		Input/output 3	
1 (+)	2 (-)	26 (B)	27 (A)	24 (+)	25 (-)	22 (+)	23 (-)
Device-specific terminal assignment: adhesive label in terminal cover.							

Modbus RS485

Supply voltage		Input/output 1		Input/output 2		Input/output 3	
1 (+)	2 (-)	26 (B)	27 (A)	24 (+)	25 (-)	22 (+)	23 (-)
Device-specific terminal assignment: adhesive label in terminal cover.							


PROFINET

Supply voltage		Input/output 1	Input/output 2		Input/output 3	
1 (+)	2 (-)	PROFINET (RJ45 connector)	24 (+)	25 (-)	22 (+)	23 (-)
Device-specific terminal assignment: adhesive label in terminal cover.						

EtherNet/IP

Supply voltage		Input/output 1	Input/output 2		Input/output 3	
1 (+)	2 (-)	EtherNet/IP (RJ45 connector)	24 (+)	25 (-)	22 (+)	23 (-)
Device-specific terminal assignment: adhesive label in terminal cover.						

Remote display and operating module DKX001

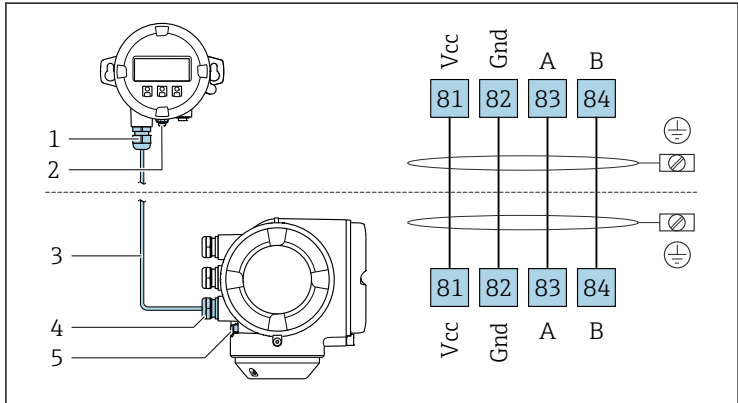

A0027518

- 1 Remote display and operating module DKX001
- 2 Protective earth (PE)
- 3 Connecting cable
- 4 Measuring device
- 5 Protective earth (PE)

Safety-related values

Order code for "Output; input 1"	Output type	Safety-related values "Output; input 1"	
		26 (+)	27 (-)
Option BA	Current output 4 to 20 mA HART	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$	
Option GA	PROFIBUS PA	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$	
Option LA	PROFIBUS DP	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$	
Option MA	Modbus RS485	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$	
Option SA	FOUNDATION Fieldbus	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$	
Option NA	EtherNet/IP	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$	
Option RA	PROFINET	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$	

Order code for "Output; input 2"; "Output; input 3"	Output type	Safety-related values			
		Output; input 2		Output; input 3	
		24 (+)	25 (-)	22 (+)	23 (-)
Option B	Current output 4 to 20 mA	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$			
Option D	User-configurable input/output	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$			
Option E	Pulse/frequency/ switch output	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$			
Option F	Double pulse output	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$			
Option H	Relay output	$U_N = 30 V_{DC}$ $I_N = 100 mA_{DC}/500 mA_{AC}$ $U_M = 250 V_{AC}$			
Option I	Current input 4 to 20 mA	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$			
Option J	Status input	$U_N = 30 V_{DC}$ $U_M = 250 V_{AC}$			

Intrinsically safe values

Order code for "Output; input 1"	Output type	Intrinsically safe values "Output; input 1"	
		26 (+)	27 (-)
Option HA	PROFIBUS PA Ex i (STANDARD + FISCO)	Ex ic $U_i = 32 \text{ V}$ $I_i = 570 \text{ mA}$ $P_i = 8.5 \text{ W}$ $L_i = 10 \text{ } \mu\text{H}$ $C_i = 5 \text{ nF}$	
Option TA	FOUNDATION Fieldbus Ex i (STANDARD + FISCO)	Ex ic $U_i = 32 \text{ V}$ $I_i = 570 \text{ mA}$ $P_i = 8.5 \text{ W}$ $L_i = 10 \text{ } \mu\text{H}$ $C_i = 5 \text{ nF}$	

Order code for "Output; input 2"; "Output; input 3"	Output type	Intrinsically safe values			
		Output; input 2		Output; input 3	
		24 (+)	25 (-)	22 (+)	23 (-)
Option C	Current output 4 to 20 mA Ex i passive	$U_i = 30 \text{ V}$ $I_i = 100 \text{ mA}$ $P_i = 1.25 \text{ W}$ $L_i = 0$ $C_i = 0$			
Option G	Pulse/frequency/ switch output Ex i passive	$U_i = 30 \text{ V}$ $I_i = 100 \text{ mA}$ $P_i = 1.25 \text{ W}$ $L_i = 0$ $C_i = 0$			

Remote display DKX001

Basic specification, position 1, 2 Approval	Terminal assignment	Basic specification, position 8 Display; Operation Option O
Option NS	81, 82, 83, 84	$U_n = 3.3 \text{ V}$
		$I_n = 150 \text{ mA}$



71561035

www.addresses.endress.com
